

1
2
3 Individualized body geometry correction factor (K_B)
4 for use when predicting body composition from bioimpedance spectroscopy
5

6 Leigh C. Ward¹, Jonathon C.K. Wells², Jaz Lyons-Reid³ and Mya T. Tint^{4,5}
7
8
9

10 ¹ School of Chemistry and Molecular Biosciences, The University of Queensland, Brisbane, Australia

11
12 ² University College London Great Ormond Street Institute of Child Health, London, UK
13

14 ³ Liggins Institute, University of Auckland, Auckland, New Zealand.
15

16 ⁴ Singapore Institute for Clinical Sciences, Agency for Science, Technology and Research (A*STAR),
17 Singapore.
18
19

20
21 ⁵ Human Potential Translational Research Programme, Yong Loo Lin School of Medicine, National
22 University of Singapore, Singapore
23
24
25

26
27 Running title: Individualized K_B
28

29 Address for correspondence: Hon A/Prof LC Ward
30

31 School of Chemistry and Molecular Biosciences,
32

33 The University of Queensland
34

35 St Lucia, Brisbane
36

37 Australia 4072
38

39 Email: l.ward@uq.edu.au
40

41 Phone: +61 7 4317 331 167
42

43 FAX: +61 7 33654699
44
45

46 **Conflict of interest**
47

48 Author Ward consults to ImpediMed Ltd., manufacturer of impedance devices. ImpediMed Ltd. had no
49 involvement in the concept, design or execution of these study nor in the preparation of the manuscript.
50
51

52 All other authors have no relevant conflicts of interest to report.
53
54
55
56
57
58
59
60

ABSTRACT (250 words)

Objective: Prediction of body composition from bioimpedance spectroscopy (BIS) measurements using mixture theory-based biophysical modelling invokes a factor (K_B) to account for differing body geometry (or proportions) between individuals. To date, a single constant value is commonly used. The aim of this study was to investigate variation in K_B across individuals and to develop a procedure for estimating an individualized K_B value.

Approach: Publicly available body dimension data, primarily from the garment industry, were used to calculate K_B values for individuals of varying body sizes across the life-span. The 3-D surface relationship between weight, height and K_B , was determined and used to create look-up tables to enable estimation of K_B in individuals based on height and weight. The utility of the proposed method was assessed by comparing fat-free mass predictions from BIS using either a constant K_B value or the individualized value.

Results: Computed K_B values were well fitted to height and weight by a 3-D surface ($R^2 = 0.988$). Body composition was predicted more accurately compared to reference methods when using individualized K_B than a constant value in infants and children but improvement in prediction was less in adults particularly those with high body mass index.

Significance: Prediction of body composition from BIS and mixture theory is improved by using an individualized body proportion factor in those of small body habitus, e.g. children. Improvement is small in adults or non-existent in those of large body size. Further improvements may be possible by incorporating a factor to account for trunk size, i.e., waist circumference.

1. Introduction

Bioelectrical impedance technologies have become increasingly popular for the assessment of human body composition *in vivo* (Ward 2021). Bioelectrical impedance analysis (BIA) methods fall into two categories: estimation of body composition based on empirically-derived prediction equations for total body water (TBW) (Kyle *et al* 2004b, 2004a) or fat-free mass (FFM), or estimations based on a biophysical model derived from mixture theory. originally developed by Hanai to describe the electrical properties of emulsions ((Hanai 1968) Mixture theory subsequently formed the basis of a biophysical model to describe the relationship between the body's electrical impedance (or resistance) and body water volumes, TBW and its sub-compartments intra- and extracellular water (ICW and ECW respectively) (De Lorenzo *et al* 1997) and comprehensively reviewed by Matthie (Matthie 2008). The first approach typically uses electrical resistance measured at a single or few frequencies (single- or multi-frequency bioelectrical impedance analysis; SFBIA, MFBIA respectively) while the second adopts a spectroscopic approach (bioelectrical impedance spectroscopy, BIS) measuring resistance over a range of frequencies and using Cole modelling to estimate resistance at zero and infinite frequencies representative of ECW and TBW respectively (Ward *et al* 2015a, Stahn *et al* 2012, Cornish *et al* 1993) and then applying these measured resistances in the mixture theory-based biophysical model. The algorithms underpinning this biophysical model are complex and have been described in detail elsewhere (Ward *et al* 2015a, Stahn *et al* 2012). Irrespective of which approach is adopted, BIA is based on the relationships that, for a homogeneous uniform cylindrical conductor, resistance is proportional to conductor length and inversely proportional to cross-sectional area. From these relationships and simple geometry of a cylinder yields

$$Volume = \rho \frac{L^2}{R} \quad \dots[1]$$

where L = conductor length (cm); R = resistance (ohm) and ρ is the specific resistivity of the conductive volume (ohm.cm). Clearly, application of this model to the human body is problematic since the body is neither homogeneous nor a simple cylinder. The biophysical model attempts to account for this by

1
2 assuming homogeneity of the body water compartments and that body consists of five inter-connected
3
4 cylinders representing the trunk and the four limbs.
5

6
7 De Lorenzo et al. attempted to account for the complex cylindrical geometry (interconnected segments
8
9 of the leg, trunk and arm in wrist-ankle impedance measurements) of the human body by modifying
10
11 Equation 1 to include a body proportion factor, K_B , that relates to the relative proportions of the leg, arm
12
13 and torso (Equation 2) (De Lorenzo *et al* 1997)
14
15

$$16 \quad \text{Volume} = K_B \rho \frac{L^2}{R} \quad \dots[2]$$

17
18
19
20 K_B can be calculated from anthropometric measurements (segment lengths and girths) and a value of 4.3,
21
22 originally determined by de Lorenzo et al. (De Lorenzo *et al* 1997), is commonly used. This value was
23
24 determined from anthropometric measurements obtained from United States army personnel (De
25
26 Lorenzo *et al* 1997, Gordon *et al* 1989). The assumption of applicability of this value to all populations
27
28 irrespective of individual body habitus has, however, been criticized as incorrect and contributing to
29
30 inaccuracy in estimations of body composition when using mixture theory (Kagawa *et al* 2014, Cox-Reijven
31
32 and Soeters 2000, Cox-Reijven *et al* 2002, Ward *et al* 2015a, Moissl *et al* 2006, Jødal 2010, Ward *et al*
33
34 1998). This is highlighted when the biophysical approach is used to estimate body composition in babies
35
36 where a K_B value of 3.8 was found to be more appropriate (Collins *et al* 2013), while values of up to 6.5
37
38 have been observed in the obese (Cox-Reijven and Soeters 2000). This has led to a call for personalization
39
40 of K_B parameters used in BIS and mixture theory prediction of body composition (Seoane *et al* 2015). The
41
42 aims of the present study were to assess the range of K_B observed in the general population across a range
43
44 of body habitus from birth to adulthood and to develop a procedure for estimating an individualized K_B
45
46 value based upon simple anthropometric measurements of height and weight.
47
48
49
50
51
52
53
54
55
56
57
58
59
60

2. Methods

2.1. Source data

Anthropometric data were primarily extracted from standard tables of body measurements provided by American Society for Testing and Materials (ASTM) International primarily for use in the apparel industry (Godil and Ressler 2008). Data are available in a number of separate ASTM standards for both sexes across the lifespan (Supplemental Table 1). The tables of data are constructed from various data sources including U.S. Department of Commerce through (ASTM International 1971) and subsequent reports, the Caesar Study (Robinette *et al* 2003), the SizeUSA study (TC2 2006), various CDC Anthropometric Reference Data reports, e.g. (McDowell *et al* 2009) according to internationally recognized principles on standardization and defined in ASTM-defined standard D5219 (ASTM International 2015a). The data provided vary slightly for different population groups but included all body dimensions to calculate K_B , i.e. arm length and circumference, leg length and circumference, and trunk length and circumference in addition to height or crown-heel length for babies. Standards are generally presented in both SI (metric) and inch-pound units; where only inch-pound units were available, data were converted to metric equivalents. Data are provided as population mean values stratified by garment size (US) within each body size category used within the garment industry, e.g., “Misses Petite”, “Misses tall”, “Boys” etc.

ASTM standards data for babies and infants are sparse. Additional data were sourced primarily from the studies of Merlob and colleagues (Merlob *et al* 1983, 1986, Sivan *et al* 1984, Merlob *et al* 1984) and Kwok *et al.* (Kwok *et al* 2007). Additional data was obtained from a sub-study of the Growing Up in Singapore Towards healthy Outcomes (GUSTO) study (Tint *et al* 2016). A total of 344 individual data sets were available for analysis.

2.2 Calculation of K_B

The body proportion coefficient, K_B , was calculated using the formula described by de Lorenzo et al (De Lorenzo *et al* 1997):

$$K_B = \frac{1}{L^2} \left[\left(\frac{L_l}{C_l^2} + \frac{L_t}{C_t^2} + \frac{L_a}{C_a^2} \right) (2L_a C_a^2 + 2L_l C_l^2 + L_t C_t^2) \right] \quad \dots[3]$$

where L = length (cm); C = circumference (cm) and subscripts indicate body region: t = trunk, l = leg and a = arm. Leg length was assumed equivalent to ASTM-designated “crotch height”; trunk length equivalent to ASTM-designated “cervicale to crotch height” and arm length equivalent to ASTM-designated “underarm length” (ASTM International 2015a). Circumference values were calculated as the mean of ASTM-designated chest and waist girths for the trunk, mid-thigh and ankle girths for the leg and mean of upper arm and wrist girths for the arm. Detailed description of terminology and diagrams showing anatomical sites of measurement for these data are provided in (ASTM International 2015a). Body volume (excluding hands, feet and head) was also calculated from these dimensions assuming cylindrical geometry for body segments as for the calculation of K_B . Height and weight were also extracted from the available data. Weight was not provided for four data sets and hence was imputed using a regression equation for calculated body volume against weight for data sets where weight was available.

2.3. Relationship of K_B with height and weight

The relationship between height, weight and K_B was explored based on treating the data as a set of three-dimensional points. Height and weight represented a two-dimensional X-Z grid with K_B plotted as the Y values in the vertical dimension. Three-D surface mesh plots for the irregularly spaced data were produced using NCSS version 10.0.10 (NCSS Statistical Software. NCSS, LLC. Kaysville, Utah, USA, ncss.com/software/ncss). Separate plots were prepared for males and female infants. Surface fitting of the data was accomplished using the automated fitting routines of Table Curve 3D and the Watson

1
2 interpolation algorithm to a uniform grid (Table Curve 3D version 4 Systat software, San Jose, California).
3
4 Separate plots were prepared for males and female infants. Surface fitting of the data was accomplished
5
6 using the automated fitting routines of Table Curve 3D and the Watson interpolation algorithm to a
7
8 uniform grid.
9
10

11 12 13 14 15 **2.4. Prediction of K_B from height and weight**

16
17 TableCurve3D version 4.0.05 (Systat Software Inc., San Jose) was used to create interpolated values from
18
19 the modelled surface at 5 kg (from 5 to 200 kg) and 5 cm (from 5 to 200 cm) intervals for each sex
20
21 separately. The resulting height, weight, K_B data matrices was exported to Excel to provide 2-dimensional
22
23 look-up data tables. The predicted K_B value for a given height and weight data pair can be calculated from
24
25 these data tables using the Excel bilinear interpolation function, InterpolateXY (Stelling Consulting, Alphen
26
27 aan den Rijn, The Netherlands).
28
29
30
31
32
33
34

35 **2.5. Performance assessment of individualized K_B values in prediction of body composition**

36
37 Body composition was predicted from BIS data for existing data sets for 4.5-month-old infants (Lingwood
38
39 *et al* 2012); children aged 6.5 to 9.5 years (Al-Ati *et al* 2015, Ward *et al* 2015b); overweight and obese
40
41 adolescents aged 10 to 18 years (Wan *et al* 2014) and healthy adults aged 18 to 49 years from the 1999-
42
43 2000 NHANES survey (National Center for Health Statistics 2012). Although different impedance devices
44
45 were used in each of these studies [ImpediMed SFB7 (Lingwood *et al* 2012, Al-Ati *et al* 2015, Ward *et al*
46
47 2015b); Tanita MC-180MA, (Wan *et al* 2014); Xitron Hydra 4200 (National Center for Health Statistics
48
49 2012)] each provided the requisite impedance data for use in the biophysical body composition model –
50
51 resistance at zero frequency (R_0) and resistance at infinite frequency (R_{inf}). The reader is referred to the
52
53 primary source citation for full methodological information. In order to facilitate comparison, these raw
54
55
56
57
58
59
60

1
2 resistance data were analysed with the same biophysical model software (Bioimp BatchBCA version
3
4 1.4.0.0, ImpediMed Ltd., Brisbane, Australia) as described previously ((Ward *et al* 2015a) using the same
5
6 parameters ($\rho_i = 1018$ and 1023.5 ohm.cm and $\rho_e = 309.9$ and 316.1 ohm.cm for males and females
7
8 respectively, body density (D_b) = 1.05 g/mL and hydration fraction of 0.732) as described previously
9
10 (Ward *et al* 2015a) except for K_B which was either set as a fixed value (group F) of 4.3 (De Lorenzo *et al*
11
12 1997) or the individualized values (group I) derived as described above (section 2.4). For infants (data of
13
14 Lingwood *et al* 2012), hydration fraction was individualized according to Fomon *et al.* (Fomon *et al* 1982)
15
16 and these data were additionally analysed using BIS parameters determined for neonates (group F2) by
17
18 Collins *et al.* (Collins *et al* 2013). Data comparison was based upon predicted fat-free mass (FFM) and was
19
20 compared to reference FFM from the original source data.
21
22
23
24
25
26
27

28 **2.6 Statistical analysis**

29
30
31 Normality of data was assessed using Kolmogorov-Smirnov test. Since K_B was not normally distributed,
32
33 comparison of calculated and imputed K_B values was performed using Passing and Bablok regression that
34
35 makes no assumptions about the underlying data distributions. Agreement between FFM predicted by BIS
36
37 using either fixed K_B or individualized K_B values was assessed by concordance correlation, limits of
38
39 agreement (LOA) analysis and determination of median absolute percentage error (MAPE). All statistical
40
41 analyses were performed with either MedCalc[®] Statistical Software version 20.013 (MedCalc Software
42
43 Ltd, Ostend, Belgium; <https://www.medcalc.org>; 2021) or JASP version 0.15 (University of Amsterdam,
44
45 <https://jasp-stats.org>). Surface fitting was accomplished using Table Curve 3D version 4.0.05 (Systat
46
47 Software Inc., Richmond, USA, <https://systat.com>) and plotted using either Slidewrite v7.01 (Advanced
48
49 Graphics Software, Rancho Santa Fe, USA) or NCSS v10.0.10 (NCSS LLC. Kaysville, USA
50
51 <https://ncss.com/software/ncss>).
52
53
54
55
56
57
58
59
60

3. RESULTS

3.1 Anthropometric characteristics of K_B -data sources

The distributions of height and weight for participants within each data set are presented in Figure 1.

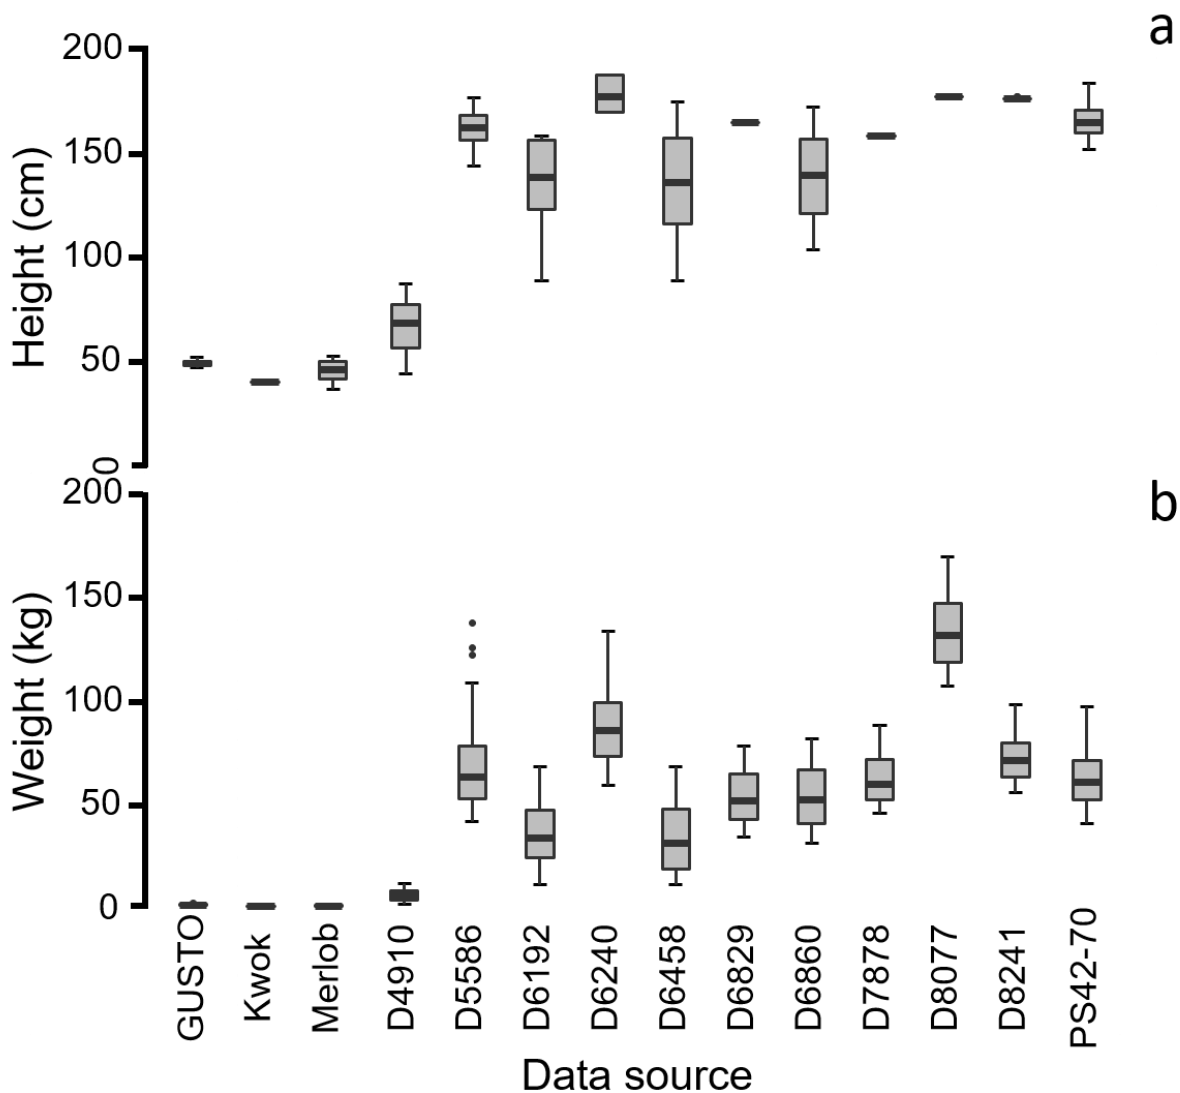


Figure 1. Distributions of height (Panel a) and weight (Panel b) for each data source. Box plots represent the median as the central line, the first and third quartiles as the edges of the box, 1.5 x the interquartile range above and below the box as lines and outliers beyond these bounds as symbols (•).

1
2 Height (crown-heel supine length for babies) ranged from 35.8 to 188 cm with weight ranging from 1.6 to
3
4 170.1 kg (Table 1).
5

6
7 TABLE 1 HERE
8
9

10
11
12 Both height and weight were bi-modally distributed with, notably relative fewer data in the 60 to 130 cm
13 height and 15 to 40 kg weight ranges reflecting few school-aged children in the data sets (Supplemental
14
15 Data Figure 1).
16
17
18
19
20
21
22
23
24
25
26
27
28
29
30
31
32
33
34
35
36
37
38
39
40
41
42
43
44
45
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60

Table 1. General characteristics of source data for generation of K_B values²

Data source ¹	Group	Sex	Age (y)	N ³	Height (cm)	Weight (kg)	BMI (kg/m ²)	K_B
ASTM D5586 (ASTM International 2002)	“Junior”, “Junior petite”, “Petite”, “Misses” & “Misses tall”	Female	>55	47	161.9 ± 8.3 (144.1 – 177.3)	70.0 ± 22.6 (43.0 – 138.2)	26.4 ± 7.1 (17.9 – 51.7)	4.0 ± 0.4 (3.6 – 5.4)
ASTM D6829 (ASTM International 2015b)	“Juniors”	Female	na ⁴	11	165.1	54.9 ± 14.6 (35.3 – 79.2)	20.2 ± 5.3 (13.7 – 29.1)	3.7 ± 0.4 (3.2 – 4.3)
ASTM D7878 (ASTM International 2013)	“Misses petite”	Female	na	24	158.7	63.7 ± 13.1 (46.8 – 89.0)	25.3 ± 5.2 (18.6 – 35.3)	4.0 ± 0.1 (3.8 – 4.2)
ASTM D6192 (ASTM International 2019b)	“Regular”, “slim” & “Plus”	Female	<12.5	34	136.2 ± 20.6 (88.9 – 158.7)	37.4 (12.1 – 69.1)	19.1 ± 3.6 (14.0 – 27.8)	4.0 ± 0.1 (3.8 – 4.3)
ASTM D6240 (ASTM International 2021)	“Mature”	Male	>35	48	178.6 ± 7.4 (170.2 – 188.0)	88.6 ± 18.8 (60.3 – 134.1)	27.8 ± 5.9 (18.7 – 41.9)	4.0 ± 0.3 (3.3 – 4.6)
ASTM D6458 (ASTM International 2019c)	“Boys Slim” & “Regular”	Male	< 15	24	136.5 ± 26.2 (88.9 – 175.3)	35.5 ± 17.7 (12.1 – 69.1)	16.5 ± 2.5 (12.5 – 20.7)	4.0 ± 0.1 (3.8 – 4.1)
ASTM D8077 (ASTM International 2016)	“Mature large”	Male	na	7	177.8	135.0 ± 22.0 (107.8 – 170.1)	42.7 ± 6.9 (34.1 – 53.8)	4.7 ± 0.1 (4.6 – 4.8)

Table 1 continued. General characteristics of source data for generation of K_B values²

Data source ¹	Group	Sex	Age (y)	N ³	Height (cm)	Weight (kg)	BMI (kg/m ²)	K_B
ASTM D8241 (ASTM International 2019d)	“Young men”	Male	na	14	176. ± 8.5 (176.5 – 177.8)	73.7 ± 12.9 (56.5 – 99.0)	23.6 ± 4.0 (18.1 – 31.3)	3.9 ± 0.3 (3.5 – 4.6)
ASTM D4910 (ASTM International 2019a)	Neonate & Infants	Combined	Birth to 2	8	66.9 ± 15.2 (44.4 – 87.6)	7.5 ± 1.2 (2.8 – 12.7)	16.5 ± 2.1 (12.6 – 18.6)	3.2 ± 2.8 (2.8 3.4)
PS42-70 (ASTM International 1971)	“Junior”, “Junior petite”, “Petite”, “Misses” & “Misses tall”	Female	na	37	161.3 ± 8.7 (147.3 – 179.1)	57.7 ± 14.2 (35.5 – 129.3)	22.0 ± 3.7 (15.7 – 30.0)	4.40 ± 0.2 (3.6 – 4.4)
GUSTO (Tint <i>et al</i> 2016)	Neonate	Male	Birth	23	48.0 ± 1.4 (46.0 – 51.0)	2.8 ± 0.3 (2.3 – 3.8)	12.1 ± 1.3 (10.2 – 14.7)	2.1 ± 0.3 (1.7 _ 2.8)
		Female		7	48.3 ± 1.8 (46.0 – 50.5)	2.9 ± 0.2 (2.6 – 3.1)	12.3 ± 0.6 (11.3 – 13.2)	2.3 ± 0.4 (1.7 – 2.8)
Kwok (Kwok <i>et al</i> 2007)	Neonate	Female	Birth	1	39.4	2.0	8.8	2.9
Merlob (Merlob <i>et al</i> 1984, Sivan <i>et al</i> 1984, Merlob <i>et al</i> 1983)	Neonate	Male	Birth	15	45.3 ± 4.8 (37.3 – 51.4)	2.1 ± 0.4 (1.6 – 2.1)	10.7 ± 2.0 (8.0 – 13.3)	1.9 ± 0.1 (1.7 _ 2.1)
		Female		15	44.5 ± 5.0 (35.8 – 50.4)	2.1 ± 0.4 (1.6 – 2.7)	10.6 ± 2.0 (7.3 – 13.2)	1.9 ± 0.2 (1.4 – 2.2)

¹See Supplemental Data Table 1 for details of source data. ²See Supplemental Table 2 for detailed anthropometric data used to generate K_B .

³N=number of data points used, actual contributing participant numbers are larger (see Supplemental Data Table 1). ⁴Not available. Data are presented as mean ± SD (range).

3.2 Computation of K_B

A bimodal distribution was also observed for K_B reflecting the similar distribution for height and weight (Supplemental Figure 2). K_B values ranged from 1.26 to 5.43. The 3-D surface distributions of K_B with height and weight are presented in Figure 2. Optimal surface fitting (maximum likelihood estimation) was achieved with Chebyshev cosine series bivariate 10th order polynomial (coefficient of determination $R^2 = 0.988$). Similar surfaces were found for both males and females with generally larger K_B values associated with larger height-weight combinations. Neither surface was a smooth flat plane with a small but apparent peak at low weight-high length combinations. Surfaces were well fitted (coefficient of determination $R^2 = 0.988$) and there was a strong correlation ($r^2 = 0.930$, $SEE = 0.207$, $P < 0.0001$) between K_B calculated according to Equation 3 and values imputed from the 3-D surfaces (Figure 3).

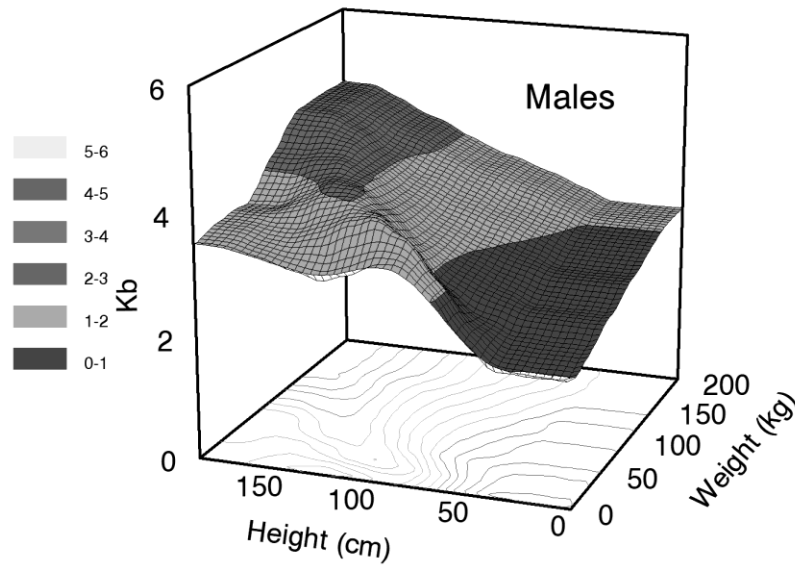
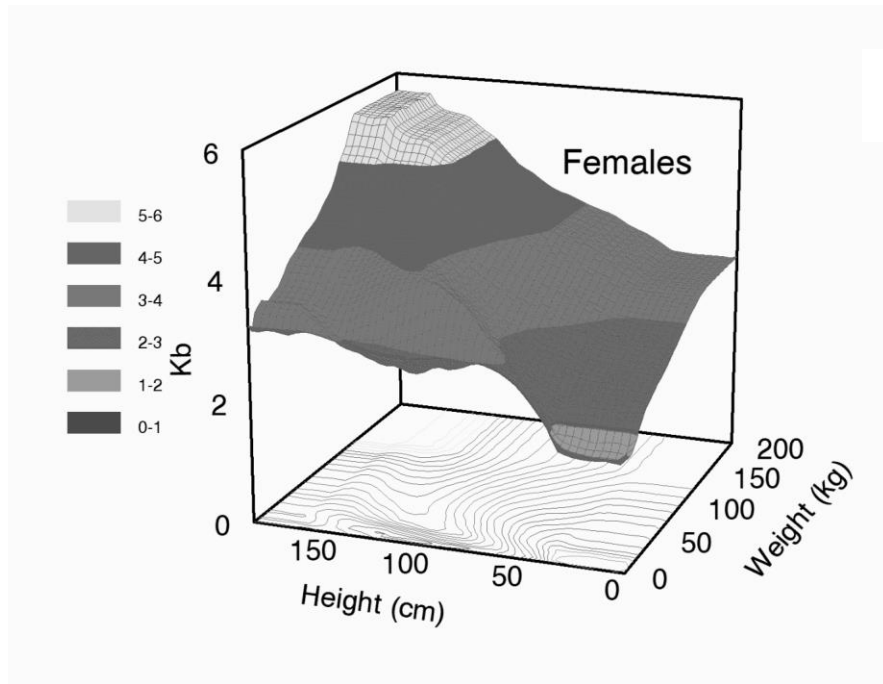


Figure 2. Three-dimensional surface plots of the relationship between height and weight and K_B

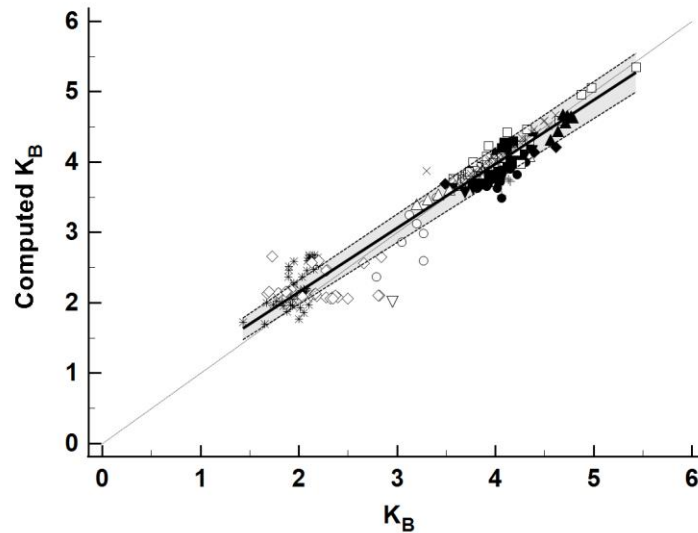


Figure 3. Relationship between calculated K_B from anthropometric parameters and the computed K_B from the 3-D surfaces. Data are presented as a Passing-Bablok regression with the line of best fit shown (—) overlaid on the line of identity (—). The shaded region represents the 95% confidence interval range. Individual data sources are represented by different symbols: \times D6240, $+$ D6458, \blacksquare D7878, \square D5586, \blacklozenge D8241, \bullet D6192, \diamond Gusto, \triangle D6829, ∇ Kwok, \blacktriangle D8077, \blacktriangledown PS42-70, $*$ Merlob, \circ D4910 (see Supplemental Data Table 1 for details).

3.3 Comparison of individual and fixed K_B values for predicting body composition.

K_B values calculated from heights and weights for the comparison studies are presented in Table 2.

TABLE 2 HERE

There were approximately equal numbers of males and females in each cohort with cohort sizes ranging from 22 to 758 participants. Heights ranged from 61 (4.5 m infants) to 199.4 cm (adults) and weights from 5.4 to 144.5 kg with BMI values ranging from 12.3 to a maximum of 57.5 kg/m². Computed K_B values ranged from 2.5 to 5.5, generally increasing from neonates to high BMI adults (Table 2). Fat-free masses were smallest, not unexpectedly, for neonates with a minimum of 4.2 kg and the largest, 94.4 kg, for adults. Generally, FFM was overestimated by BIS compared to measured values. Overestimation was largest when a fixed K_B value was used and decreased by between 1.6 kg in neonates and 4.3 kg adult males (BMI 20-25 kg/m²) when individualized K_B values were used. Improvement in prediction with the

1
2 use of individualized K_B was, however, limited to those participants with BMI values below 30 (WHO
3 classification of overweight or below). Indeed in those participants with BMI values >30, i.e. WHO
4 classification as obese, use of individual K_B values worsened prediction (Table 2). This was confirmed by
5 lower MAPE values for the BMI <30 cohorts for individualized K_B calculations but higher MAPE values in
6 the BMI >30 groups. Despite the improvement in population, mean prediction (smaller bias compared to
7 measured FFM) by the use of individual K_B in the lower BMI groups there was no difference in the LOA.
8
9 For neonates, the use of resistivity coefficients specific for neonates (Collins *et al* 2013) improved
10 prediction compared to conventional fixed K_B BIS but this improvement was still less than that observed
11 when individualized K_B values were used.
12
13
14
15
16
17
18
19
20
21
22
23
24
25
26
27
28
29
30
31
32
33
34
35
36
37
38
39
40
41
42
43
44
45
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60

Table 2. Comparison of prediction of body composition using either a fixed value for K_B (F and F2) or individualised values (I).

Source Reference	Group	Sex Number	Height (cm)	Weight (kg)	BMI ¹ (kg/m ²)	K_B	FFM ² (kg)	K_B type	Predicted FFM (kg)	1.96 SD Limits of Agreement	MAPE ³ (%)	
(Lingwood <i>et al</i> 2012)	Infants (4.5 months)	Female	66.2 ± 2.3	7.2 ± 0.9	16.5 ± 1.8	3.0 ± 0.06	5.4 ± 0.5	F	6.8 ± 1.1	-2.7 – 0.0	26.4	
		N = 25	(62.2 – 69.6)	(5.4 – 8.9)	(13.8 – 20.5)	(2.9 – 3.1)	(4.3 – 6.3)	F2	6.0 ± 0.9	-1.7 – 0.6	11.7	
									I	5.2 ± 0.9	-0.8 – 1.3	5.4
		Male	64.5 ± 1.1	7.0 ± 0.6	16.7 ± 1.3	2.7 ± 0.07	4.9 ± 0.3	F	6.2 ± 0.9	-2.9 – 0.2	24.0	
		N = 25	(61.0 – 67.7)	(5.9 – 8.0)	(13.9 – 19.4)	(2.5 – 2.8)	(4.2 – 5.6)	F2	5.8 ± 0.9	-2.5 – 0.5	16.4	
									I	4.6 ± 0.7	-1.0 – 1.5	10.0
(Ward <i>et al</i> 2015b)	6.5 – 9.5 years	Female	129.8 ± 6.4	33.9 ± 10.8	19.8 ± 5.1	3.9 ± 0.1	21.1 ± 3.9	F	23.6 ± 5.1	-5.7 – 0.8	11.2	
		N = 75	(113.9 – 148.8)	(19.1 – 65.5)	(13.6 – 35.2)	(3.7 – 4.1)	(14.5 – 36.5)	I	21.0 ± 4.8	-2.8 – 3.2	4.5	
		Male	129.0 ± 7.4	33.6 ± 11.1	19.8 ± 4.7	3.9 ± 0.1	19.9 ± 4.4	F	22.5 ± 5.6	-6.0 – 0.8	12.5	
		N = 83	(112.2 – 149.5)	(18.2 – 76.5)	(13.5 – 35.7)	(3.6 – 4.2)	(13.0 – 36.8)	I	20.2 ± 5.4	-3.4 – 2.8	5.2	
Wan (Wan <i>et al</i> 2014)	10 – 17 years	Female	159.6 ± 8.9	83.9 ± 19.7	32.5 ± 6.60	4.3 ± 0.3	43.0 ± 8.1	F	49.9 ± 9.5	-12.0 – 1.8	15.5	
		N = 29	(144.0 – 178.0)	(49.9 – 129.9)	(22.8 – 47.7)	(3.9 – 95.2)	(31.1 – 63.8)	I	50.1 ± 12.0	-16.1 – 1.9	16.8	
		Male	165.3 ± 11.9	95.1 ± 21.0	34.6 ± 5.6	4.2 ± 0.2	52.8 ± 13.5	F	59.6 ± 14.4	-13.2 – -0.4	12.9	
		N = 29	(139.0 – 186.0)	(56.7 – 128.6)	(21.9 – 48.6)	(3.9 – 4.6)	(27.0 – 80.0)	I	59.4 ± 15.7	-14.7 – 1.4	13.2	

¹BMI= body mass index. ²FFM = fat-free mass. ³MAPE = median absolute percentage error. F = fixed K_B value = 4.3; F2 = fixed K_B value = 3.8. I = individualized K_B value.

Table 2 continued. Comparison of prediction of body composition using either a fixed value for K_B (F and F2) or individualised values (I).

Source Reference	Group	Sex Number	Height (cm)	Weight (kg)	BMI ¹ (kg/m ²)	K_B	FFM ² (kg)	K_B type	Predicted FFM (kg)	1.96 SD Limits of Agreement	MAPE ³ (%)
NHANES (National Center for Health Statistics 2012)	BMI <19.9	Female N = 74	161.0 ± 6.7 (145.6 – 174.5)	42.9 ± 11.6 (19.1 – 71.1)	18.5 ± 1.2 (14.8 – 20.0)	4.2 ± 0.3 (3.7 – 4.7)	35.1 ± 4.0 (26.5 – 46.2)	F I	37.3 ± 4.3 36.5 ± 4.3	-6.0 – 1.6 -6.8 – 4.0	7.3 5.5
		Male N = 513	154.6 ± 17.1 (115.8 – 192.5)	48.1 ± 5.0 (39.3 – 59.8)	17.6 ± 1.6 (12.3 – 20.0)	3.7 ± 0.07 (3.6 – 3.9)	34.7 ± 10.6 (14.3 – 59.3)	F I	37.6 ± 11.0 34.2 ± 9.9	-7.0 – 1.2 -3.8 – 4.7	8.9 3.9
	BMI 20-24.9	Female N = 311	162.6 ± 6.9 (143.3 – 180.4)	60.3 ± 6.4 (42.8 – 80.2)	22.7 ± 1.4 (20.0 – 24.9)	3.9 ± 0.06 (3.8 – 4.2)	40.0 ± 4.5 (26.6 – 54.0)	F I	43.7 ± 5.1 41.0 ± 5.0	-8.6 – 1.1 -5.8 – 3.7	9.5 4.4
		Male N = 758	168.4 ± 12.5 (126.7 – 199.4)	64.0 ± 10.3 (34.0 – 88.7)	22.4 ± 1.4 (20.0 – 24.9)	3.8 ± 0.08 (3.6 – 4.0)	50.1 ± 10.1 (19.8 – 74.9)	F I	54.3 ± 10.6 50.2 ± 9.6	-9.9 – 1.4 -6.0 – 5.7	9.1 4.1
	BMI 25-29.9	Female N = 250	161.7 ± 6.6 (154.3 – 179.4)	71.5 ± 7.2 (55.2 – 91.9)	27.3 ± 1.5 (25.0 – 29.9)	4.0 ± 0.06 (4.0 – 4.3)	43.4 ± 4.8 (31.0 – 57.5)	F I	48.2 ± 5.7 46.3 ± 5.7	-9.9 – 0.5 -8.1 – 2.3	10.9 6.7
		Male N = 519	171.9 ± 9.7 (132.0 – 197.5)	80.9 ± 10.1 (45.3 – 108.4)	27.3 ± 1.4 (25.0 – 29.9)	4.0 ± 0.08 (3.9 – 4.3)	58.6 ± 4.8 (25.6 – 81.3)	F I	64.3 ± 10.1 61.5 ± 10.0	-12.6 – 1.3 -9.8 – 4.0	9.8 5.2
	BMI 30-39.9	Female N = 257	160.6 ± 7.1 (133.0 – 178.4)	88.1 ± 11.6 (65.5 – 125.5)	34.1 ± 2.8 (30.0 – 39.9)	4.3 ± 0.02 (4.1 – 5.2)	49.2 ± 6.3 (34.9 – 67.1)	F I	55.3 ± 7.2 55.4 ± 8.3	-13.1 – 0.9 -14.1 – 1.7	12.5 12.4
		Male N = 290	174.2 ± 8.8 (143.5 – 196.0)	101.7 ± 13.4 (62.0 – 134.4)	33.4 ± 2.5 (30.0 – 39.9)	4.3 ± 0.2 (4.1 – 4.7)	68.3 ± 10.0 (37.1 – 94.4)	F I	75.3 ± 11.4 75.4 ± 12.7	-15.9 – 1.9 -17.3 – 3.1	9.7 9.7
	BMI >40	Female N = 56	161.2 ± 6.3 (145.3 – 172.8)	114.7 ± 11.7 (89.8 – 144.5)	44.1 ± 3.4 (40.0 – 57.5)	4.8 ± 0.2 (4.4 – 5.5)	58.9 ± 6.2 (46.8 – 72.1)	F I	68.1 ± 7.9 73.5 ± 10.4	-18.8 – 0.5 -26.8 – -2.4	14.7 23.5
		Male N = 22	170.8 ± 5.1 (162.8 – 178.6)	124.8 ± 7.1 (111.3 – 138.1)	42.8 ± 2.1 (40 – 48.2)	4.5 ± 0.08 (4.4 – 4.6)	75.1 ± 6.3 (62.3 – 88.4)	F I	82.8 ± 8.8 85.7 ± 9.6	-18.8 – 3.3 -22.5 – 1.3	9.4 12.8

¹BMI= body mass index. ²FFM = fat-free mass. ³MAPE = median absolute percentage error. F = fixed K_B value = 4.3; F2 = fixed K_B value = 3.8. I = individualized K_B value.

4. DISCUSSION

The present study has demonstrated that the use of a body proportion factor (K_B) personalized to the individual improves prediction of body composition from BIS data. This improvement was only seen in those individuals with BMI $<30 \text{ kg/m}^2$. Conventional whole body, wrist to ankle, impedance measurements assumes that the body conforms to a simple single cylindrical geometry, which is clearly not the case. The body proportion factor attempts to account for the relative differences between the body segments (leg, trunk and arm) in shape and size. A value of $K_B = 4.3$ is commonly used irrespective of body habitus. Although it has been recognized previously that this value will not adequately represent relative body proportions in all individuals (Cox-Reijven *et al* 2002) and that K_B varies markedly between individuals even in a relatively homogeneous group of adults (Ward *et al* 2015a), little attempt has been made to correct for potential error introduced by use of an inaccurate K_B . Two approaches have been attempted. Firstly, Moissl (Moissl *et al* 2006) introduced a modification to BIS and mixture theory, termed BCS, body composition spectroscopy, that corrected the mixture theory equations according to the subjects BMI. While this approach has merit, its effectiveness is questionable in some populations (Ellegård *et al* 2009). The second approach has been to measure the impedance of each of the body segments separately and to calculate whole body composition from the segmental data (Ward 2012). The wide-spread adoption of this method has, however, been driven primarily by the development of the stand-on impedance analyser rather than to mitigate body shape errors in whole-body measurements. Notably, most of these devices are not BIS devices but single or multi-frequency devices that predict body composition from empirically-derived population-specific algorithms not mixture theory (Ward 2012).

It is feasible to personalize K_B for each individual by obtaining the required anthropometric measurements and using Equation 3. In practice this is unlikely to be adopted due to the logistics and time involved in obtaining the requisite anthropometric measurements. Furthermore, anthropometric measurements are susceptible to considerable measurement error and specially trained anthropometrists are required (Perini *et al* 2005). An

1
2 alternative is to approximate K_B for an individual based on more readily obtainable measurements that relate
3
4 closely to body shape and size. In the present study, an individualized K_B value was derived as a function of weight
5
6 and height rather than from the more time-consuming approach of obtaining the necessary anthropometric
7
8 dimensional measurements. The approach adopted in the present study is conceptually similar to that used
9
10 previously in using simply height and weight, but rather than using these combined as a single correction factor,
11
12 BMI (Moissl *et al* 2006), each was used independently to predict K_B from the relationship between all three
13
14 variables determined in a calibration population. This approach assumes that a relationship between K_B , weight
15
16 and height exists, and varies in a systematic manner as body shape and size varies. This hypothesis was supported
17
18 by the observations of the present study that change in K_B with height and weight could be well represented by
19
20 a surface plane, which could be used as a calibration surface to estimate a K_B value for height-weight pairs. The
21
22 relationship between K_B as the independent variable and height and weight as predictor variable could not be
23
24 adequately represented by a multiple regression equation since this procedure assumes a perfectly flat surface.
25
26
27
28
29
30
31

32
33 Although prediction of K_B from height and weight was shown to have merit improving prediction of body
34
35 composition in those with BMI $<30 \text{ kgm}^2$, the method is clearly imperfect. Height and weight alone or combined
36
37 as in BMI are not reflective of body shape or the relative masses/volumes of the body segments. Once adulthood
38
39 is achieved, height changes very little decreasing slightly but progressively as one ages. Weight, on the other
40
41 hand, varies markedly between individuals or within individuals over the life-span, or with disease and nutritional
42
43 change. Accumulation or loss of body mass generally does not occur proportionally across the body segments.
44
45 Accumulation of body fat may occur as increased appendicular subcutaneous adipose tissue or increased visceral
46
47 and abdominal adipose mass; under these conditions two individuals with the same body mass would have
48
49 different relative proportions of trunk to appendicular volume and K_B despite the same height-weight
50
51 combination. This would not be detected by the present method, instead both would be predicted to have
52
53 identical K_B values.
54
55
56
57
58
59
60

1
2
3
4
5 This confounding effect is most likely to be observed in those who are overweight or obese. Data from the
6 present study provides support for this view. Body (excluding hands feet and head) and segment volumes were
7 calculated from the anthropometric data for the K_B data sets. Segment volumes were computed assuming simple
8 cylindrical geometry from the circumferential and length data for the body segments. There was no difference
9 in trunk volume as a proportion of total volume for those with BMI < 25 kg/m² but from there on, relative trunk
10 volume increased progressively as BMI increased (Figure 4). This suggests that as BMI increased K_B prediction
11 would become progressively more inaccurate. This is reflected in individualized K_B values having no advantage
12 over a fixed value of 4.3 when predicting FFM (Table 2). It is possible that a correction factor could be applied
13 based on measurement of waist circumference as an index of increased trunk volume. Although this would
14 require an extra measurement when using BIS, this is unlikely to be an onerous imposition since waist
15 circumference is frequently measured in clinical practice in body composition studies (Ross *et al* 2020) although
16 its accuracy has been questioned (Verweij *et al* 2013).
17
18
19
20
21
22
23
24
25
26
27
28
29
30
31
32
33
34
35
36
37
38
39
40
41
42
43
44
45
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60

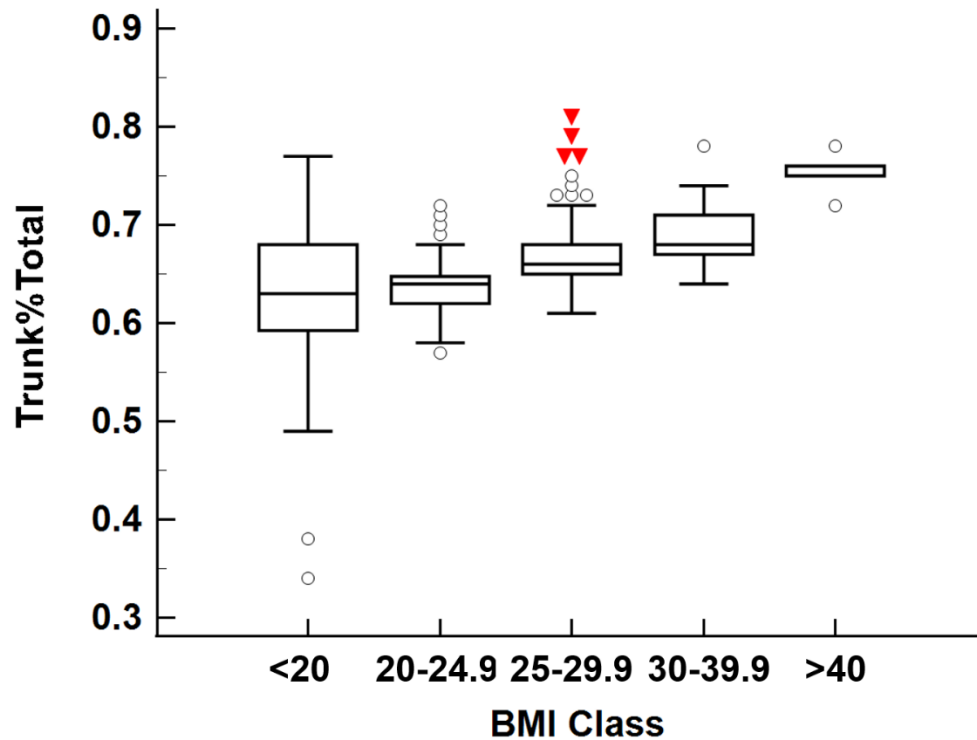


Figure 4. Change in relative volumes of the trunk and total body in individuals in the K_B data set (see Supplemental Data Table 1 for details).

A number of limitations to the study should be acknowledged. K_B values were calculated from readily available anthropometric data. These data were primarily sourced from anthropometric measurements used to derive standards for body sizing in the garment industry. These data are exclusively obtained from surveys undertaken in the general population of the USA. In addition, while the exact number of individuals providing data are unknown, the ASTM data are designed to be representative of the population. As such, they may not be a good reflection of other populations with notably different body habitus, for example Asian. Although the ASTM standards are updated regularly, they continue to include data from earlier decades. This problem of old data was also apparent in that other than the studies of Merlob there appear to be no single studies in neonates in which all the required measurements are available. Improvements in health and nutrition over this time could

1
2 potentially mean that the data used here do not reflect well contemporary populations. Precise methodological
3
4 details for measurement methods are lacking but it is assumed that data were obtained in accordance with ASTM
5
6 recommendations (ASTM International 2015a). Comparatively few data were available for infants and children,
7
8 particularly with heights between 60 and 130 cm. The inadequacies of the current data could potentially be
9
10 addressed by the use of data available from large surveys of populations using 3-D laser scanning (Koepke *et al*
11
12 2017, Santos *et al* 2016). Potentially, it may be possible to determine K_B from segmental volumes estimated from
13
14 photographs obtained using a smartphone for an individual at the time of BIS measurement (Farina *et al* 2016,
15
16 Majola 2020).
17
18
19
20
21
22
23

24 In conclusion, this study has demonstrated the potential advantage of using personalized K_B values in mixture
25
26 theory when predicting body composition from BIS data. The method proposed, based on height and weight,
27
28 anthropometric measurements already obtained as part of the BIS protocol requires further modification to be
29
30 applicable across the broad range of body habitus seen in the human population. Improved performance may
31
32 be possible through refinement of the K_B calibration using contemporary anthropometric data from laser
33
34 scanning studies and by correction for central adiposity using waist circumference.
35
36
37
38
39
40
41
42
43
44
45
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60

1
2 Acknowledgements
3

4
5 None
6

7
8 Funding disclosure
9

10
11 None
12

13
14 Ethical permissions
15

16
17 No ethical permissions were required for this study. All data analysed has previously been published or is the
18
19 public domain with all appropriate approvals at time of data collection.
20
21
22
23
24
25
26
27
28
29
30
31
32
33
34
35
36
37
38
39
40
41
42
43
44
45
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60

REFERENCES

Al-Ati T, Preston T, Al-Hooti S, Al-Hamad N, Al-Ghanim J, Al-Khulifi F, Al-Lahou B, Al-Othman A and Davidsson L

2015 Total body water measurement using the 2 H dilution technique for the assessment of body

composition of Kuwaiti children *Public Health Nutr.* **18** 259–63 Online:

https://www.cambridge.org/core/product/identifier/S1368980013003534/type/journal_article

ASTM International 2019a *D4910/D4910M – 19 Standard Tables of Body Measurements for Children, Infant*

Sizes – Preemie to 24 Months (West Conshohocken, PA) Online:

<https://www.astm.org/Standards/D4910.htm>

ASTM International 2015a *D5219 – 15 Standard Terminology Relating to Body Dimensions for Apparel Sizing*

(West Conshohocken, PA) Online: <https://www.astm.org/Standards/D5219.htm>

ASTM International 2002 *D5586 – 01 Standard Standard Tables of of Body Measurements for Women Aged 55*

and Older (West Conshohocken, PA) Online:

<https://www.astm.org/DATABASE.CART/WITHDRAWN/D5586D5586M.htm>

ASTM International 2019b *D6192/D6192M – 19 Standard Tables of Body Measurements for Girls, Sizes 2 to 20*

(Reg & Slim) and Girls Plus (West Conshohocken, PA) Online:

<https://www.astm.org/Standards/D6192.htm>

ASTM International 2021 *D6240/D6240M – 12 Standard Tables of Body Measurements for Mature Men , ages*

35 and older , Sizes Thirty-Four to Fifty-Two (34 to 52) Short , Regular , and (West Conshohocken, PA)

Online: <https://www.astm.org/Standards/D6240.htm>

ASTM International 2019c *D6458/D6458M – 19 Standard Tables of Body Measurements for Boys, Sizes 4 to 20*

Slim and 2 to 20 Regular (West Conshohocken, PA) Online: <https://www.astm.org/Standards/D6458.htm>

ASTM International 2015b *D6829 – 02 Standard Tables of Body Measurements for Juniors, Sizes 0 to 19* (West

1
2
3 Conshohocken, PA) Online: <https://www.astm.org/Standards/D6829.htm>
4

5 ASTM International 2013 *D7878/D7878M Standard Tables for Body Measurements for Adult Female Misses*
6

7 *Petite Figure Type, Size Range 00P – 20P* (West Conshohocken, PA) Online:
8

9 <https://www.astm.org/Standards/D7878.htm>
10
11

12 ASTM International 2016 *D8077/D8077M – 16 Standard Tables for Body Measurements for Mature Big Men*
13

14 *Type, Size Range 46-64* (West Conshohocken, PA) Online: <https://www.astm.org/Standards/D8077.htm>
15
16
17

18 ASTM International 2019d *D8241/D8241M – 19 Standard Tables of Body Measurements for Young Men Type,*
19

20 *Size Range 32 – 48* (West Conshohocken, PA) Online: <https://www.astm.org/Standards/D8241.htm>
21
22

23 ASTM International 1971 *Voluntary Product Standard PS42-70 Body measurements for the sizing of women's*
24

25 *patterns and apparel* (West Conshohocken, PA, PA) Online: [http://gsi.nist.gov/global/docs/stds/womens-](http://gsi.nist.gov/global/docs/stds/womens-ps42-70.pdf)
26
27 [ps42-70.pdf](http://gsi.nist.gov/global/docs/stds/womens-ps42-70.pdf)
28
29

30 Collins C T, Reid J, Makrides M, Lingwood B E, McPhee A J, Morris S A, Gibson R A and Ward L C 2013 Prediction
31

32 of body water compartments in preterm infants by bioelectrical impedance spectroscopy *Eur. J. Clin. Nutr.*
33

34 **67** S47–53 Online: <http://dx.doi.org/10.1038/ejcn.2012.164>
35
36
37

38 Cornish B H, Thomas B J and Ward L C 1993 Improved prediction of extracellular and total body water using
39

40 impedance loci generated by multiple frequency bioelectrical impedance analysis *Phys. Med. Biol.* **38**
41

42 337–46 Online: <http://stacks.iop.org/0031-9155/38/i=3/a=001>
43
44

45 Cox-Reijven P and Soeters P 2000 Validation of bio-impedance spectroscopy: Effects of degree of obesity and
46

47 ways of calculating volumes from measured resistance values *Int. J. Obes.* **24** 271–80 Online:
48

49 <http://www.nature.com/articles/0801123>
50
51

52 Cox-Reijven P, van Kreel B and Soeters P 2002 Accuracy of bioelectrical impedance spectroscopy in measuring
53

54 changes in body composition during severe weight loss *J. Parenter. Enter. Nutr.* **26** 120–7 Online:
55
56
57
58
59
60

1
2
3 <https://onlinelibrary.wiley.com/doi/10.1177/0148607102026002120>

4
5 Ellegård L H, Åhlén M, Körner U, Lundholm K G, Plank L D and Bosaeus I G 2009 Bioelectric impedance
6 spectroscopy underestimates fat-free mass compared to dual energy X-ray absorptiometry in incurable
7 cancer patients *Eur. J. Clin. Nutr.* **63** 794–801 Online: <http://www.nature.com/articles/ejcn200835>
8
9

10
11
12 Farina G L, Spataro F, De Lorenzo A and Lukaski H 2016 A smartphone application for personal assessments of
13 body composition and phenotyping *Sensors (Switzerland)* **16** 2163 Online: [http://www.mdpi.com/1424-](http://www.mdpi.com/1424-8220/16/12/2163)
14
15
16
17
18
19 8220/16/12/2163

20 Fomon S J, Haschke F, Ziegler E E and Nelson S E 1982 Body composition of reference children from birth to age
21 10 years. *Am. J. Clin. Nutr.* **35** 1169–75 Online: <http://www.ncbi.nlm.nih.gov/pubmed/7081099>
22
23
24

25 Godil A and Ressler S 2008 Shape and Size Analysis and Standards *Handbook of Digital Human Modeling*
26
27
28 *Research for Applied Ergonomics and Human Factors Engineering* pp 14-1-14–5 Online:
29
30
31 <http://www.crcnetbase.com/doi/abs/10.1201/9781420063523.ch14>

32 Gordon C C, Churchill T, Clauser C, Bradtmiller B, McConville J T, Tebbetts I and Walker R A 1989 1988
33
34
35
36
37
38
39
40
41
42
43
44
45
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60
ANTHROPOMETRIC SURVEY OF U.S. ARMY PERSONNEL: SUMMARY STATISTICS INTERIM REPORT (Natick,
Mass) Online: <http://oai.dtic.mil/oai/oai?verb=getRecord&metadataPrefix=html&identifier=ADA209600>

Hanai T 1968 Electrical properties of emulsions. *Emulsion science* ed P Sherman (Academic Press, London) pp
354–477.

Jødal L 2010 *Electrical theory behind the measurement of body fluids with bioimpedance spectroscopy (BIS)*
(Aalborg) Online: https://pure.au.dk/portal/files/20320521/Lecture_notes_on_BIS.pdf

Kagawa M, Wishart C and Hills A 2014 Influence of Posture and Frequency Modes in Total Body Water
Estimation Using Bioelectrical Impedance Spectroscopy in Boys and Adult Males *Nutrients* **6** 1886–98
Online: <http://www.mdpi.com/2072-6643/6/5/1886>

- 1
2
3 Koepke N, Zwahlen M, Wells J C, Bender N, Henneberg M, Rühli F J and Staub K 2017 Comparison of 3D laser-
4 based photonic scans and manual anthropometric measurements of body size and shape in a validation
5 study of 123 young Swiss men *PeerJ* **5** e2980 Online: <https://peerj.com/articles/2980>
6
7
8
9
10 Kwok Y, Wong K, Ying B, Yick K, Yi L and Chap-yung Y 2007 Anthropometric measurement of premature infants
11
12 *Int. J. Cloth. Sci. Technol.* **19** 319–33 Online:
13
14 <http://www.emeraldinsight.com/10.1108/09556220710819519>
15
16
17 Kyle U G, Bosaeus I, De Lorenzo A D, Deurenberg P, Elia M, Manuel Gómez J, Lilienthal Heitmann B, Kent-Smith
18
19 L, Melchior J-C, Pirlich M, Scharfetter H, M.W.J Schols A and Pichard C 2004a Bioelectrical impedance
20 analysis—part II: utilization in clinical practice *Clin. Nutr.* **23** 1430–53 Online:
21
22 <https://linkinghub.elsevier.com/retrieve/pii/S0261561404001633>
23
24
25
26
27 Kyle U G, Bosaeus I, Lorenzo A D De, G M, Lilienthal B, Kent-smith L, Melchior J C, Pichard C, Group W, De
28
29 Lorenzo A D, Deurenberg P, Elia M, Gómez J M, Heitmann B L, Kent-smith L, Melchior J C, Pirlich M,
30
31 Scharfetter H, Schols A M W J and Pichard C 2004b Bioelectrical impedance analysis part I: review of
32
33 principles and methods *Clin. Nutr.* **23** 1226–43 Online:
34
35
36 <https://linkinghub.elsevier.com/retrieve/pii/S0261561404000937>
37
38
39 Lingwood B E, Storm van Leeuwen A-M, Carberry A E, Fitzgerald E C, Callaway L K, Colditz P B and Ward L C
40
41 2012 Prediction of Fat-Free Mass and Percentage of Body Fat in Neonates using Bioelectrical Impedance
42
43 Analysis and Anthropometric Measures: Validation against the PEA POD *Br. J. Nutr.* **107** 1545–52 Online:
44
45 https://www.cambridge.org/core/product/identifier/S0007114511004624/type/journal_article
46
47
48 De Lorenzo A, Andreoli A, Matthie J and Withers P 1997 Predicting body cell mass with bioimpedance by using
49
50 theoretical methods: a technological review *J. Appl. Physiol.* **82** 1542–58 Online:
51
52 <http://www.ncbi.nlm.nih.gov/pubmed/9134904>
53
54
55
56 Majola K 2020 Three-Dimensional Body Volume Measurement From Two-Dimensional Images: Towards A
57
58
59
60

1
2 Smartphone Application 81 Online: <http://hdl.handle.net/11427/32797>

3
4
5 Matthie J R 2008 Bioimpedance measurements of human body composition: Critical analysis and outlook

6
7 *Expert Rev. Med. Devices* **5** 239–61 Online: <http://www.ncbi.nlm.nih.gov/pubmed/18331184>

8
9
10 McDowell M A, Fryar C D and Ogden C L 2009 Anthropometric reference data for children and adults: United

11
12 States, 1988-1994. *Vital Health Stat. 11.* **11** 1–68 Online:

13
14 <http://www.ncbi.nlm.nih.gov/pubmed/19642512>

15
16
17 Merlob P, Sivan Y and Reisner S 1986 Ratio of crown-rump distance to total length in preterm and term infants

18
19 *J. Med. Genet.* **23** 338–40 Online: <http://jmg.bmj.com/cgi/doi/10.1136/jmg.23.4.338>

20
21
22 Merlob P, Sivan Y and Reisner S H 1984 Anthropometric measurements of the newborn infant (27 to 41

23
24 gestational weeks). *Birth Defects Orig. Artic. Ser.* **20** 1–52 Online:

25
26 <http://www.ncbi.nlm.nih.gov/pubmed/6536341>

27
28
29 Merlob P, Sivan Y, Reisner S H, Merlob P and Reisner S H 1983 Upper Limb Standards in Newborns *Am. J. Dis.*

30
31 *Child.* **137** 829–32 Online: <http://www.ncbi.nlm.nih.gov/pubmed/6613948>

32
33
34 Moissl U M, Wabel P, Chamney P W, Bosaeus I, Levin N W, Bosy-Westphal A, Korth O, Müller M J, Ellegård L,

35
36 Malmros V, Kaitwatcharachai C, Kuhlmann M K, Zhu F, Fuller N J, Manfred J M, Kaitwatcharachai C,

37
38 Kuhlmann M K and Zhu F 2006 Body fluid volume determination via body composition spectroscopy in

39
40 health and disease *Physiol. Meas.* **27** 921–33 Online: <https://iopscience.iop.org/article/10.1088/0967->

41
42 [3334/27/9/012](https://iopscience.iop.org/article/10.1088/0967-3334/27/9/012)

43
44
45
46
47 National Center for Health Statistics 2012 *National Health and Nutrition Examination Survey (NHANES), 1999-*

48
49 *2000* Online: <https://wwwn.cdc.gov/nchs/nhanes/1999-2000/BIX.htm>

50
51
52 Perini T A, Oliveira G L de, Ornellas J dos S and Oliveira F P de 2005 Cálculo do erro técnico de medição em

53
54 antropometria *Rev. Bras. Med. do Esporte* **11** 81–5 Online:

1
2 http://www.scielo.br/scielo.php?script=sci_arttext&pid=S1517-86922005000100009&lng=pt&tlng=pt

3
4
5 Robinette K M, Daanen H and Paquet E 2003 The CAESAR project: a 3-D surface anthropometry survey *Second*
6
7 *International Conference on 3-D Digital Imaging and Modeling (Cat. No.PR00062)* (IEEE Comput. Soc) pp
8
9 380–6 Online: <http://ieeexplore.ieee.org/document/805368/>

10
11
12 Ross R, Neeland I J, Yamashita S, Shai I, Seidell J, Magni P, Santos R D, Arsenault B, Cuevas A, Hu F B, Griffin B A,
13
14 Zambon A, Barter P, Fruchart J-C, Eckel R H, Matsuzawa Y and Després J-P 2020 Waist circumference as a
15
16 vital sign in clinical practice: a Consensus Statement from the IAS and ICCR Working Group on Visceral
17
18 Obesity. *Nat. Rev. Endocrinol.* **16** 177–89 Online: <http://www.ncbi.nlm.nih.gov/pubmed/32020062>

19
20 Santos L P, Ong K K, Day F, Wells J C K, Matijasevich A, Santos I S, Victora C G and Barros A J D 2016 Body shape
21
22 and size in 6-year old children: assessment by three-dimensional photonic scanning *Int. J. Obes.* **40** 1012–
23
24 7 Online: <http://dx.doi.org/10.1038/ijo.2016.30>

25
26
27 Seoane F, Abtahi S, Abtahi F, Ellegård L, Johannsson G, Bosaeus I and Ward L C 2015 Mean Expected Error in
28
29 Prediction of Total Body Water: A True Accuracy Comparison between Bioimpedance Spectroscopy and
30
31 Single Frequency Regression Equations *Biomed Res. Int.* **2015** 1–11 Online:
32
33 <http://www.hindawi.com/journals/bmri/2015/656323/>

34
35
36 Sivan Y, Reisner S H, Merlob P, Sivan Y, Reisner S H, Merlob P, Sivan Y and Reisner S H 1984 Lower Limb
37
38 Standards in Newborns *Am. J. Dis. Child.* **138** 140–2 Online:
39
40 <http://www.ncbi.nlm.nih.gov/pubmed/6695869>

41
42
43 Stahn A, Terblanche E and Gunga H 2012 Selected Applications of Bioelectrical Impedance Analysis: Body
44
45 Fluids, Blood Volume, Body Cell Mass and Fat Mass *Handbook of Anthropometry* ed V R Preedy (New
46
47 York, NY, NY: Springer New York) pp 415–40 Online: [http://link.springer.com/10.1007/978-1-4419-1788-](http://link.springer.com/10.1007/978-1-4419-1788-1_23)
48
49
50
51
52
53
54
55
56
57
58
59
60
1_23

TC2 2006 SizeUSA US National Sizing Survey Online: <https://www.tc2.com/size-usa.html>

- 1
2
3 Tint M-T, Ward L C, Soh S E, Aris I M, Chinnadurai A, Saw S M, Gluckman P D, Godfrey K M, Chong Y-S, Kramer
4 M S, Yap F, Lingwood B and Lee Y S 2016 Estimation of fat-free mass in Asian neonates using bioelectrical
5 impedance analysis *Br. J. Nutr.* **115** 1033–42 Online:
6
7 https://www.cambridge.org/core/product/identifier/S0007114515005486/type/journal_article
8
9
10
11 Verweij L M, Terwee C B, Proper K I, Hulshof C T and van Mechelen W 2013 Measurement error of waist
12 circumference: gaps in knowledge *Public Health Nutr.* **16** 281–8 Online:
13
14 https://www.cambridge.org/core/product/identifier/S1368980012002741/type/journal_article
15
16
17
18
19 Wan C S, Ward L C, Halim J, Gow M L, Ho M, Briody J N, Leung K, Cowell C T and Garnett S P 2014 Bioelectrical
20 impedance analysis to estimate body composition, and change in adiposity, in overweight and obese
21 adolescents: comparison with dual-energy x-ray absorptiometry *BMC Pediatr.* **14** 249 Online:
22
23 [http://www.pubmedcentral.nih.gov/articlerender.fcgi?artid=4288657&tool=pmcentrez&rendertype=abst](http://www.pubmedcentral.nih.gov/articlerender.fcgi?artid=4288657&tool=pmcentrez&rendertype=abstract)
24
25
26
27
28
29
30
31
32 Ward L C 2021 Electrical bioimpedance: from the past to the future *J. Electr. Bioimpedance* **12** 1–2 Online:
33
34 <https://www.sciendo.com/article/10.2478/joeb-2021-0001>
35
36
37 Ward L C 2012 Segmental bioelectrical impedance analysis *Curr. Opin. Clin. Nutr. Metab. Care* **15** 424–9 Online:
38
39 <http://journals.lww.com/00075197-201209000-00005>
40
41
42 Ward L C, Elia M and Cornish B H 1998 Potential errors in the application of mixture theory to multifrequency
43 bioelectrical impedance analysis *Physiol. Meas.* **19** 53–60 Online:
44
45 <https://iopscience.iop.org/article/10.1088/0967-3334/19/1/005>
46
47
48
49 Ward L C, Isenring E, Dyer J M, Kagawa M and Essex T 2015a Resistivity coefficients for body composition
50 analysis using bioimpedance spectroscopy: effects of body dominance and mixture theory algorithm
51
52 *Physiol. Meas.* **36** 1529–49 Online: <http://dx.doi.org/10.1088/0967-3334/36/7/1529>
53
54
55
56 Ward L, Al Lahou B, Al Khulaifi F, Al Ghanim J and Al-Hooti S 2015b Validation of bioimpedance spectroscopy
57
58
59
60

1
2 (BIS) for body composition assessment in Kuwaiti children *Eur. J. Clin. Nutr.* **69** S34 Online:

3
4
5 <https://www.nature.com/articles/ejcn2015190>
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20
21
22
23
24
25
26
27
28
29
30
31
32
33
34
35
36
37
38
39
40
41
42
43
44
45
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60